

DiAgam

Your expert in specific proteins


CATALOGUE

AU® Chemistry Systems by Beckman Coulter

AU®480-680

AU®400-640-2700-5400

AU®5800





Company profile

MISSION STATEMENT

«To have a perfect control of Development, Manufacturing process & Selling of In Vitro Diagnostic liquid reagents with a strong focus on our Customer vision»

Your R&D Partner

DiAgam manufactures **reagents for immunoturbidimetry**.

Our company specializes in high technology R&D, based on immunology technologies. DiAgam is the creator of liquid laboratory reagents containing **gold particles**.

We are currently taking part in a project to develop **new nanotechnologies** based on the use of **colloidal particles** in the field of medical diagnosis. This activity has also succeeded in completing our products range with Cystatin C, Ferritin & Rheumatoid factor.

Manufacturer of ready-to-use reagents

All our products are developed and manufactured within the company.

Our reagents, controls and calibrators are liquid, stable and ready to use on **all opened biochemistry analyzers even with barcodes** (Abbott - Alinity – Architect , Beckman Coulter – AU series, IDS-iSYS Multi-Discipline Automated System, Menarini – Zenit RA, Mindray BS series, Ortho - VITROS® 5,1 FS Chemistry, VITROS® 4600 Chemistry, VITROS® 5600 Integrated Systems, Roche - Modular®-COBAS C, Siemens - Advia® 1800 - Advia® 2400 - Atellica®, Thermo-Konelab®, etc...)

DiAgam is a member of the National Association of **European Diagnostic Manufacturers Association (EDMA)**. All reagents are labelled and DiAgam is certified **ISO 9001:2015** and **ISO 13485:2016**.

All calibrators and controls are traceable to the **International Standards** (WHO, IFCC, NIBSC, etc.)

Worldwide reliability

DiAgam promotes its products in B to B and B to C businesses through its direct affiliates in Belgium, France and Iberia. We also export in ASEAN, EMAE, Americas.

Thanks to our **manufacturing flexibility**, we can propose all our parameters in three different packagings: **Kits** especially dedicated to particular analyzers, **Vials** filled and **Bulk**, available under **DiAgam** label or in **OEM**.


We respect our philosophy by offering our customer, a **high quality of our products** with a most **competitive price** along with a continuous quest to **satisfy their needs**.

ALBUMIN
ALPHA 1 - ACID GLYCOPROTEIN
ALPHA 1 - ANTITRYPSIN
ALPHA 1 - MICROGLOBULIN
ALPHA 2 - MACROGLOBULIN
ANTITHROMBIN III
APOLIPOPROTEIN A1
APOLIPOPROTEIN B
ASO

BETA 2 - MICROGLOBULIN
CALPROTECTIN (new)
CERULOPLASMIN
C3
C4
CRP
CYSTATIN C
FERRITIN
FIBRINOGEN
HAPTOGLOBIN

Ig A
Ig E (new)
Ig G
Ig M
LIPOPROTEIN A
MICROALBUMIN
PREALBUMIN
RETINOL BINDING PROTEIN
RHEUMATOID FACTOR
TRANSFERRIN



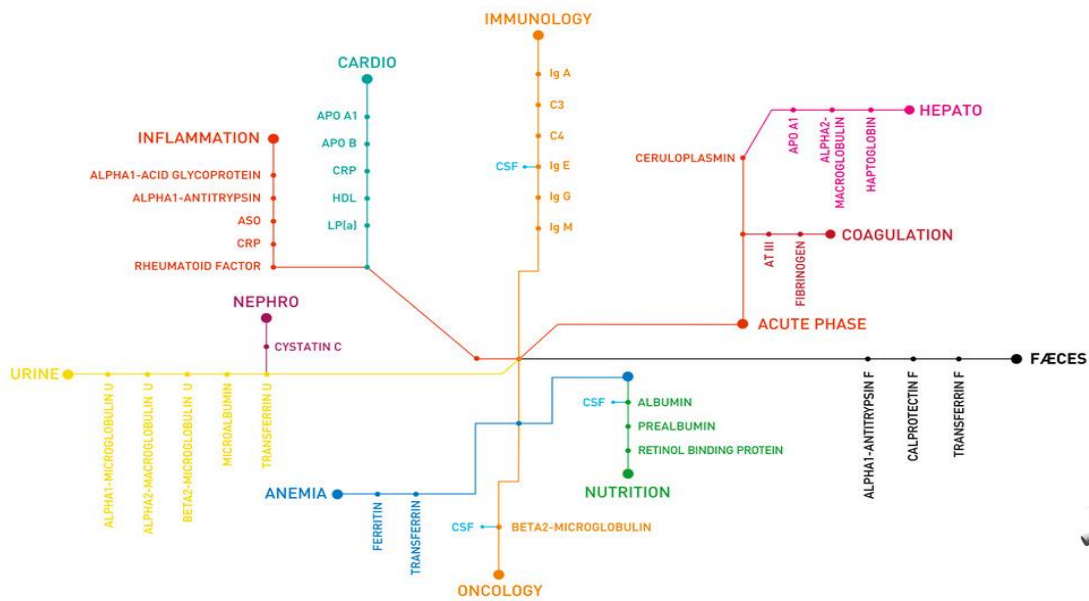

CATALOGUE - AU® Chemistry Systems

New

Calprotectin

REAGENTS	<i>Reference</i>	<i>Content</i>	<i>Shelf Life*</i>	<i>Sample**</i>	<i>Analytical Range***</i>	<i>Tests****</i>
-----------------	------------------	----------------	--------------------	-----------------	----------------------------	------------------

Please contact us for more information

CALPROTECTIN TEST

New

SARS-CoV-2 SEROLOGICAL ASSAY

REAGENTS	<i>Reference</i>	<i>Content</i>	<i>Shelf Life*</i>	<i>Sample**</i>	<i>Analytical Range***</i>	<i>Tests****</i>
-----------------	------------------	----------------	--------------------	-----------------	----------------------------	------------------

Please contact us for more information

SARS-CoV-2 SEROLOGICAL ASSAY based on PETIA Colloidal Gold

CATALOGUE - AU® Chemistry Systems

ALBUMIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	ALTUR-B00/AU	1x50 ml	1x15 ml	36 months	Serum and plasma	1,096 - 120.44 (g/l)	417
	ALTUR-H00/AU	2x50 ml	2x15 ml				833
	ALTUR-L00/AU	12x50 ml	12x15 ml				5000
KIT for AU®400-640-2700-5400	ALTUR-B00/AU	1x50 ml	1x15 ml	36 months	Serum and plasma	1,096 - 120.44 (g/l)	222
	ALTUR-H00/AU	2x50 ml	2x15 ml				444
	ALTUR-L00/AU	12x50 ml	12x15 ml				2667
KIT for AU®5800	ALTUR-B00/AU	1x50 ml	1x15 ml	36 months	Serum and plasma	1,096 - 120.44 (g/l)	510
	ALTUR-H00/AU	2x50 ml	2x15 ml				1020
	ALTUR-L00/AU	12x50 ml	12x15 ml				6122

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

ALBUMIN CSF

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	CSF	10,86 - 494,33 (mg/l)	417
	MATUR-H00/AU	2x50 ml	2x10 ml				833
	MATUR-L00/AU	12x50 ml	12x10 ml				5000
KIT for AU®400-640-2700-5400	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	CSF	10,86 - 494,33 (mg/l)	333
	MATUR-H00/AU	2x50 ml	2x10 ml				667
	MATUR-L00/AU	12x50 ml	12x10 ml				4000
KIT for AU®5800	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	CSF	10,86 - 494,33 (mg/l)	556
	MATUR-H00/AU	2x50 ml	2x10 ml				1111
	MATUR-L00/AU	12x50 ml	12x10 ml				6667

CALIBRATORS

KIT 5 LEV	MAREK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

H	MACOZ-002	1x2 ml	18 months
H	MACOX-002	1x2 ml	18 months
M	MACON-002	1x2 ml	18 months
L	MACOS-002	1x2 ml	18 months

CATALOGUE - AU® Chemistry Systems

ALPHA-1 GLYCOPROTEIN ACIDE/OROSOMUCOID

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	GPTUR-B00/AU	1x70 ml	1x14 ml	36 months	Serum	0,143 - 2,42 (g/l)	350
	GPTUR-H00/AU	2x70 ml	2x14 ml				700
KIT for AU®400-640-2700-5400	GPTUR-B00/AU	1x70 ml	1x14 ml	36 months	Serum	0,143 - 2,42 (g/l)	280
	GPTUR-H00/AU	2x70 ml	2x14 ml				560
KIT for AU®5800	GPTUR-B00/AU	1x70 ml	1x14 ml	36 months	Serum	0,143 - 2,42 (g/l)	467
	GPTUR-H00/AU	2x70 ml	2x14 ml				933

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

ALPHA-1 ANTITRYPSIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	ATTUR-H00/AU	1x60 ml	1x12 ml	24 months	Serum and plasma	0.007 - 3.50 (g/l)	300
KIT for AU®400-640-2700-5400	ATTUR-H00/AU	1x60 ml	1x12 ml	24 months	Serum and plasma	0.007 - 3.50 (g/l)	240
KIT for AU®5800	ATTUR-H00/AU	1x60 ml	1x12 ml	24 months	Serum and plasma	0.007 - 3.50 (g/l)	400

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

ALPHA-1 MICROGLOBULIN (URINE)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®400-480-640-680-2700-5400-5800	A1DGX-B00/AU	1 x 15 ml	1 x 15 ml	6 months	Serum and plasma	1,29 - 166,6 (mg/l)	250
	A1DGX-H00/AU	2 x 20 ml	2 x 20 ml				667
	A1DGX-L00/AU	12 x 20 ml	12 x 20 ml				4000

CALIBRATORS

KIT 5 LEV	A1REK-000	5x1 ml	6 months
-----------	-----------	--------	----------

CONTROLS

M	A1CON-002	1x2 ml	6 months
L	A1COS-002	1x2 ml	6 months

CATALOGUE - AU® Chemistry Systems

ALPHA-2 MACROGLOBULIN - ALPHA-2 MACROGLOBULIN URINARY

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	MGTUR-H00/AU	1x70 ml	1x14 ml	36 months	Serum and plasma or urine	0,026 - 4,96 (g/l) serum 3,36 - 199 (mg/l) urine	350
	MGTUR-L00/AU	12x70 ml	12x14 ml				4200
KIT for AU®400-640-2700-5400	MGTUR-H00/AU	1x70 ml	1x14 ml	36 months	Serum and plasma or urine	0,026 - 4,96 (g/l) serum 3,36 - 199 (mg/l) urine	280
	MGTUR-L00/AU	12x70 ml	12x14 ml				3360
KIT for AU®5800	MGTUR-H00/AU	1x70 ml	1x14 ml	36 months	Serum and plasma or urine	0,026 - 4,96 (g/l) serum 3,36 - 199 (mg/l) urine	467
	MGTUR-L00/AU	12x70 ml	12x14 ml				5600

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months
URINARY LOW	MGCU1-002	1x2 ml	12 months
URINARY HIGH	MGCU2-002	1x2 ml	12 months

ANTI STREPTOLYSIN O (ASO)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	ASLTX-B00/AU	1x65 ml	1x7.5 ml	20 months	Serum and plasma	19.99 to 864.85 (IU/ml)	341
	ASLTX-H00/AU	2x65 ml	2x7.5 ml				682
KIT for AU®400-640-2700-5400	ASLTX-B00/AU	1x65 ml	1x7.5 ml	20 months	Serum and plasma	19.99 to 864.85 (IU/ml)	278
	ASLTX-H00/AU	2x65 ml	2x7.5 ml				556
KIT for AU®5800	ASLTX-B00/AU	1x65 ml	1x7.5 ml	20 months	Serum and plasma	19.99 to 864.85 (IU/ml)	464
	ASLTX-H00/AU	2x65 ml	2x7.5 ml				929

CALIBRATORS

H	ASREK-000	1x1 or (1x5) ml	12 months
---	-----------	-----------------	-----------

CONTROLS

M	ASCN-002	1x2 ml	12 months
---	----------	--------	-----------

CATALOGUE - AU® Chemistry Systems

ANTITHROMBIN III

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	A3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Plasma	28,15 - 806,3 (mg/l)	417
	A3TUR-H00/AU	2x50 ml	2x10 ml				833
KIT for AU®400-640-2700-5400	A3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Plasma	28,15 - 806,3 (mg/l)	333
	A3TUR-H00/AU	2x50 ml	2x10 ml				667
KIT for AU®5800	A3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Plasma	28,15 - 806,3 (mg/l)	556
	A3TUR-H00/AU	2x50 ml	2x10 ml				1111

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

APOLIPOPROTEIN A1

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	AATUR-B00/AU	1x50 ml	1x13 ml	36 months	Serum and plasma	0,029 - 4 (g/l)	245
	AATUR-H00/AU	2x50 ml	2x13 ml				491
KIT for AU®400-640-2700-5400	AATUR-B00/AU	1x50 ml	1x13 ml	36 months	Serum and plasma	0,029 - 4 (g/l)	197
	AATUR-H00/AU	2x50 ml	2x13 ml				394
KIT for AU®5800	AATUR-B00/AU	1x50 ml	1x13 ml	36 months	Serum and plasma	0,029 - 4 (g/l)	325
	AATUR-H00/AU	2x50 ml	2x13 ml				650

CALIBRATORS

KIT 5 LEV	ABREK-000	5x0,05 ml	18 months
-----------	-----------	-----------	-----------

CONTROLS

H	ABCOX-002	1x2 ml	18 months
M	ABCN-002	1x2 ml	18 months

CATALOGUE - AU® Chemistry Systems

APOLIPOPROTEIN B

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	ABTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.019 - 4 (g/l)	286
	ABTUR-H00/AU	2x50 ml	2x10 ml				571
KIT for AU®400-640-2700-5400	ABTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.019 - 4 (g/l)	200
	ABTUR-H00/AU	2x50 ml	2x10 ml				400
KIT for AU®5800	ABTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.019 - 4 (g/l)	333
	ABTUR-H00/AU	2x50 ml	2x10 ml				667

CALIBRATORS

KIT 5 LEV	ABREK-000	5x0,05 ml	18 months
H	ABREH-001 or 005	1x1 or (1x5) ml	18 months

CONTROLS

H	ABCOX-002	1x2 ml	18 months
M	ABCON-002	1x2 ml	18 months

BETA-2 MICROGLOBULIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range	Tests****
		R1	R2				
KIT for AU®480-680	B2DGX-B00/AU	1x18 ml	1x8 ml	15 months	serum and plasma	0,132 to 95 (mg/l)	125
	B2DGX-H00/AU	2x44 ml	2x19 ml				594
	B2DGX-L00/AU	8x44 ml	8x19 ml				2375
KIT for AU®400-640-2700-5400	B2DGX-B00/AU	1x18 ml	1x8 ml	15 months	serum and plasma	0,132 to 95 (mg/l)	100
	B2DGX-H00/AU	2x44 ml	2x19 ml				475
	B2DGX-L00/AU	8x44 ml	8x19 ml				1900
KIT for AU®5800	B2DGX-B00/AU	1x18 ml	1x8 ml	15 months	serum and plasma	0,132 to 95 (mg/l)	167
	B2DGX-H00/AU	2x44 ml	2x19 ml				792
	B2DGX-L00/AU	8x44 ml	8x19 ml				3167

CALIBRATORS

KIT 5 LEV	B2REK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

H	B2COX-001	1 x 1 ml	18 months
M	B2CON-003	1x3 ml	18 months
L	B2COS-003	1x3 ml	18 months

CATALOGUE - AU® Chemistry Systems

BETA-2 MICROGLOBULIN (URINE)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range	Tests****
		R1	R2				
KIT for AU®480-680	BUDGX-B00/AU	1 x 28 ml	1 x 12 ml	15 months	Urine	0,055 to 9.3 (mg/l)	125
	BUDGX-H00/AU	2 x 28 ml	2 x 12 ml				594
KIT for AU®400-640-2700-5400	BUDGX-B00/AU	1 x 28 ml	1 x 12 ml	15 months	Urine	0,055 to 9.3 (mg/l)	100
	BUDGX-H00/AU	2 x 28 ml	2 x 12 ml				475
KIT for AU®5800	BUDGX-B00/AU	1 x 28 ml	1 x 12 ml	15 months	Urine	0,055 to 9.3 (mg/l)	167
	BUDGX-H00/AU	2 x 28 ml	2 x 12 ml				792

CALIBRATORS

KIT 5 LEV	BUREK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

M	B2CON-003	1x3 ml	18 months
L	B2COS-003	1x3 ml	18 months

CERULOPLASMIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	CETUR-B00/AU	1x30 ml	1x6 ml	36 months	Serum or plasma	9,48 - 1051,2 (mg/l)	250
	CETUR-H00/AU	1x60 ml	1x12 ml				500
KIT for AU®400-640-2700-5400	CETUR-B00/AU	1x30 ml	1x6 ml	36 months	Serum or plasma	9,48 - 1051,2 (mg/l)	200
	CETUR-H00/AU	1x60 ml	1x12 ml				400
KIT for AU®5800	CETUR-B00/AU	1x30 ml	1x6 ml	36 months	Serum or plasma	9,48 - 1051,2 (mg/l)	333
	CETUR-H00/AU	1x60 ml	1x12 ml				667

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

COMPLEMENT C3

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	C3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.015 - 4.31 (g/l)	400
	C3TUR-H00/AU	2x50 ml	2x10 ml				800
KIT for AU®400-640-2700-5400	C3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.015 - 4.31 (g/l)	263
	C3TUR-H00/AU	2x50 ml	2x10 ml				526
KIT for AU®5800	C3TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0.015 - 4.31 (g/l)	500
	C3TUR-H00/AU	2x50 ml	2x10 ml				1000

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

COMPLEMENT C4

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	C4TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0,002 - 0,825 (g/l)	400
	C4TUR-H00/AU	2x50 ml	2x10 ml				800
KIT for AU®400-640-2700-5400	C4TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0,002 - 0,825 (g/l)	278
	C4TUR-H00/AU	2x50 ml	2x10 ml				556
KIT for AU®5800	C4TUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	0,002 - 0,825 (g/l)	500
	C4TUR-H00/AU	2x50 ml	2x10 ml				1000

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

CRP XL WIDE RANGE

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	CPTXL-B00/AU	1x60 ml	1x12 ml	36 months	Serum and plasma	0,607 - 425 (mg/l)	Contact us
	CPTXL-H00/AU	2x60 ml	2x12 ml				923
	CPTXL-L00/AU	12x60 ml	12x12 ml				5938
KIT for AU®400-640-2700-5400	CPTXL-B00/AU	1x60 ml	1x12 ml	36 months	Serum and plasma	0,607 - 425 (mg/l)	Contact us
	CPTXL-H00/AU	2x60 ml	2x12 ml				667
	CPTXL-L00/AU	12x60 ml	12x12 ml				4000
KIT for AU®5800	CPTXL-B00/AU	1x60 ml	1x12 ml	36 months	Serum and plasma	0,607 - 425 (mg/l)	556
	CPTXL-H00/AU	2x60 ml	2x12 ml				1111
	CPTXL-L00/AU	12x60 ml	12x12 ml				6667

CALIBRATORS

KIT 5 LEV	CPREK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

H	CPCOX-002	1x2 ml	18 months
M	CPCON-002	1x2 ml	18 months
L	CXCON-002	1x2 ml	18 months

CRP GOLD LATEX

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range	Tests****
		R1	R2				
KIT for AU®480-680	CPDGX-B00/AU	1x20 ml	1x20 ml	24 months	Serum and plasma	0,031 to 300 (mg/l)	200
	CPDGX-H00/AU	2x50 ml	2x50 ml				1000
	CPDGX-L00/AU	8x50 ml	8x50 ml				4000
KIT for AU®400-640-2700-5400	CPDGX-B00/AU	1x20 ml	1x20 ml	24 months	Serum and plasma	0,031 to 300 (mg/l)	200
	CPDGX-H00/AU	2x50 ml	2x50 ml				1000
	CPDGX-L00/AU	8x50 ml	8x50 ml				4000
KIT for AU®5800	CPDGX-B00/AU	1x20 ml	1x20 ml	24 months	Serum and plasma	0,031 to 300 (mg/l)	333
	CPDGX-H00/AU	2x50 ml	2x50 ml				1667
	CPDGX-L00/AU	8x50 ml	8x50 ml				6667

CALIBRATORS

KIT 5 LEV	CPRLK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

H	CPCOX-002	1x2 ml	18 months
M	CPCON-002	1x2 ml	18 months
L	CXCON-002	1x2 ml	18 months

CATALOGUE - AU® Chemistry Systems

CYSTATIN C - Colloidal Gold

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	CYCOL-B00/AU	1x20 ml	1x7.5 ml	6 months	Serum and plasma	0.15 to 9.355 (mg/l)	125
	CYCOL-H00/AU	2x50 ml	2x15 ml				500
	CYCOL-L00/AU	12x50 ml	12x15 ml				3000
KIT for AU®400-640-2700-5400	CYCOL-B00/AU	1x20 ml	1x7.5 ml	6 months	Serum and plasma	0.15 to 9.355 (mg/l)	100
	CYCOL-H00/AU	2x50 ml	2x15 ml				400
	CYCOL-L00/AU	12x50 ml	12x15 ml				2400
KIT for AU®5800	CYCOL-B00/AU	1x20 ml	1x7.5 ml	6 months	Serum and plasma	0.15 to 9.355 (mg/l)	167
	CYCOL-H00/AU	2x50 ml	2x15 ml				667
	CYCOL-L00/AU	12x50 ml	12x15 ml				4000

CALIBRATORS

KIT 6 LEV	CYREK-000	6x1 ml	12 months
-----------	-----------	--------	-----------

CONTROLS

M	CYCON-002	1x2 ml	12 months
---	-----------	--------	-----------

FERRITIN - Colloidal Gold

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	FNCOL-B00/AU	1x50 ml	1x9 ml	12 months	Serum	6,344 - 500 (µg/l)	360
	FNCOL-H00/AU	2x50 ml	2x9 ml				720
KIT for AU®400-640-2700-5400	FNCOL-B00/AU	1x50 ml	1x9 ml	12 months	Serum	6,344 - 500 (µg/l)	300
	FNCOL-H00/AU	2x50 ml	2x9 ml				600
KIT for AU®5800	FNCOL-B00/AU	1x50 ml	1x9 ml	12 months	Serum	6,344 - 500 (µg/l)	450
	FNCOL-H00/AU	2x50 ml	2x9 ml				900

CALIBRATORS

KIT 5 LEV	FNRGK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

M	FNCON-002	1x2 ml	18 months
---	-----------	--------	-----------

CATALOGUE - AU® Chemistry Systems

FIBRINOGEN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	FITUR-B00/AU	1x30 ml	1x6 ml	36 months	Plasma	0.05 - 10 (g/l)	250
	FITUR-H00/AU	1x60 ml	1x12 ml				500
KIT for AU®400-640-2700-5400	FITUR-B00/AU	1x30 ml	1x6 ml	36 months	Plasma	0.05 - 10 (g/l)	200
	FITUR-H00/AU	1x60 ml	1x12 ml				400
KIT for AU®5800	FITUR-B00/AU	1x30 ml	1x6 ml	36 months	Plasma	0.05 - 10 (g/l)	333
	FITUR-H00/AU	1x60 ml	1x12 ml				667

CALIBRATORS

M	FIREM-001	1x1 ml	12 months
---	-----------	--------	-----------

CONTROLS

M	FICON-001	1x1 ml	12 months
---	-----------	--------	-----------

HAPTOGLOBIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	HATUR-B00/AU	1x40 ml	1x7 ml	36 months	Serum or plasma	0.002 - 3.86 (g/l)	175
	HATUR-H00/AU	1x70 ml	1x14 ml				350
KIT for AU®400-640-2700-5400	HATUR-B00/AU	1x40 ml	1x7 ml	36 months	Serum or plasma	0.002 - 3.86 (g/l)	140
	HATUR-H00/AU	1x70 ml	1x14 ml				280
KIT for AU®5800	HATUR-B00/AU	1x40 ml	1x7 ml	36 months	Serum or plasma	0.002 - 3.86 (g/l)	233
	HATUR-H00/AU	1x70 ml	1x14 ml				467

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

IMMUNOGLOBULINS A

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	IATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.02 - 8 (g/l)	370
	IATUR-H00/AU	2x50 ml	2x10 ml				741
KIT for AU®400-640-2700-5400	IATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.02 - 8 (g/l)	299
	IATUR-H00/AU	2x50 ml	2x10 ml				599
KIT for AU®5800	IATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.02 - 8 (g/l)	500
	IATUR-H00/AU	2x50 ml	2x10 ml				1000

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

IMMUNOGLOBULINS E

NEW

[Contact us](#)

IMMUNOGLOBULINS G

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	IGTUR-B00/AU	1x50 ml	1x18 ml	36 months	Serum	0.125 - 35 (g/l)	353
	IGTUR-H00/AU	2x50 ml	2x18 ml				706
KIT for AU®400-640-2700-5400	IGTUR-B00/AU	1x50 ml	1x18 ml	36 months	Serum	0.125 - 35 (g/l)	286
	IGTUR-H00/AU	2x50 ml	2x18 ml				571
KIT for AU®5800	IGTUR-B00/AU	1x50 ml	1x18 ml	36 months	Serum	0.125 - 35 (g/l)	474
	IGTUR-H00/AU	2x50 ml	2x18 ml				947

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

IMMUNOGLOBULINS G (CSF)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	IGLCR-B00/AU	1 x 55 ml	1 x 10 ml	24 months	CSF	3,375 - 249,78 (mg/l)	667
	IGLCR-H00/AU	2 x 55 ml	2 x 10 ml				1333
KIT for AU®400-640-2700-5400	IGLCR-B00/AU	1 x 55 ml	1 x 10 ml	24 months	CSF	3,375 - 249,78 (mg/l)	667
	IGLCR-H00/AU	2 x 55 ml	2 x 10 ml				1333
KIT for AU®5800	IGLCR-B00/AU	1 x 55 ml	1 x 10 ml	24 months	CSF	3,375 - 249,78 (mg/l)	667
	IGLCR-H00/AU	2 x 55 ml	2 x 10 ml				1333

CALIBRATORS

KIT 5 LEV	IGREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	IGCOX-002	1x2 ml	24 months
M	IGCON-002	1x2 ml	24 months
L	IGCOS-002	1x2 ml	24 months

IMMUNOGLOBULINS M

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	IMTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.038 - 7 (g/l)	370
	IMTUR-H00/AU	2x50 ml	2x10 ml				741
KIT for AU®400-640-2700-5400	IMTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.038 - 7 (g/l)	299
	IMTUR-H00/AU	2x50 ml	2x10 ml				599
KIT for AU®5800	IMTUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum	0.038 - 7 (g/l)	500
	IMTUR-H00/AU	2x50 ml	2x10 ml				1000

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

LIPOPROTEIN (A)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	LPTUR2-H00/AU	1x50 ml	1x6 ml	12 months	Serum and plasma	0,0235 - 0,946 (g/l)	400
KIT for AU®400-640-2700-5400	LPTUR2-H00/AU	1x50 ml	1x6 ml	12 months	Serum and plasma	0,0235 - 0,946 (g/l)	240
KIT for AU®5800	LPTUR2-H00/AU	1x50 ml	1x6 ml	12 months	Serum and plasma	0,0235 - 0,946 (g/l)	462

CALIBRATORS

KIT 4 LEV	LPREK-000	4x0,5 ml	10 months
-----------	-----------	----------	-----------

CONTROLS

M	LPCON-002	1x2 ml	12 months
---	-----------	--------	-----------

MICROALBUMIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	Urine	1,86 - 400 (mg/l)	417
	MATUR-H00/AU	2x50 ml	2x10 ml				833
	MATUR-L00/AU	12x50 ml	12x10 ml				5000
KIT for AU®400-640-2700-5400	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	Urine	1,86 - 400 (mg/l)	333
	MATUR-H00/AU	2x50 ml	2x10 ml				667
	MATUR-L00/AU	12x50 ml	12x10 ml				4000
KIT for AU®5800	MATUR-B00/AU	1x50 ml	1x10 ml	36 months	Urine	1,86 - 400 (mg/l)	556
	MATUR-H00/AU	2x50 ml	2x10 ml				1111
	MATUR-L00/AU	12x50 ml	12x10 ml				6667

CALIBRATORS

KIT 5 LEV	MAREK-000	5x1 ml	18 months
-----------	-----------	--------	-----------

CONTROLS

H	MACOX-002	1x2 ml	18 months
M	MACON-002	1x2 ml	18 months
L	MACOS-002	1x2 ml	18 months

CATALOGUE - AU® Chemistry Systems

PREALBUMIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	PATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	6.53 - 1000 (mg/l)	370
	PATUR-H00/AU	2x50 ml	2x10 ml				741
KIT for AU®400-640-2700-5400	PATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	6.53 - 1000 (mg/l)	299
	PATUR-H00/AU	2x50 ml	2x10 ml				599
KIT for AU®5800	PATUR-B00/AU	1x50 ml	1x10 ml	36 months	Serum and plasma	6.53 - 1000 (mg/l)	500
	PATUR-H00/AU	2x50 ml	2x10 ml				1000

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months

RETINOL BINDING PROTEIN (RBP)

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	RBTUR-B00/AU	1 x 30,5 ml	1 x 10 ml	24 months	Serum or plasma	7,81 - 141 (mg/l)	400
	RBTUR-H00/AU	2 x 30,5ml	2 x 10 ml				800
	RBTUR-L00/AU	12 x 30,5 ml	12 x 10 ml				4800
KIT for AU®400-640-2700-5400	RBTUR-B00/AU	1 x 30,5 ml	1 x 10 ml	24 months	Serum or plasma	7,81 - 141 (mg/l)	400
	RBTUR-H00/AU	2 x 30,5ml	2 x 10 ml				800
	RBTUR-L00/AU	12 x 30,5 ml	12 x 10 ml				4800
KIT for AU®5800	RBTUR-B00/AU	1 x 30,5 ml	1 x 10 ml	24 months	Serum or plasma	7,81 - 141 (mg/l)	400
	RBTUR-H00/AU	2 x 30,5ml	2 x 10 ml				800
	RBTUR-L00/AU	12 x 30,5 ml	12 x 10 ml				4800

CALIBRATORS

KIT 5 LEV	RBREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	RBCOX-002	1x2 ml	24 months
M	RBCON-002	1x2 ml	24 months
L	RBCOS-002	1x2 ml	24 months

CATALOGUE - AU® Chemistry Systems

RHEUMATOID FACTOR (RF) - Colloidal Gold

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	RFCOL-B00/AU	1x50 ml	1x20 ml	18 months	Serum and plasma	2.228 - 120 (kUI/l)	230
	RFCOL-H00/AU	2x50 ml	2x20 ml				460
KIT for AU®400-640-2700-5400	RFCOL-B00/AU	1x50 ml	1x20 ml	18 months	Serum and plasma	2.228 - 120 (kUI/l)	200
	RFCOL-H00/AU	2x50 ml	2x20 ml				400
KIT for AU®5800	RFCOL-B00/AU	1x50 ml	1x20 ml	18 months	Serum and plasma	2.228 - 120 (kUI/l)	333
	RFCOL-H00/AU	2x50 ml	2x20 ml				667

CALIBRATORS

KIT 5 LEV	RFREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

M	RFCON-002	1x2 ml	24 months
---	-----------	--------	-----------

TRANSFERRIN

REAGENTS	Reference	Content		Shelf Life*	Sample**	Analytical Range***	Tests****
		R1	R2				
KIT for AU®480-680	TFTUR-H00/AU	1x70 ml	1x20 ml	36 months	Serum and plasma	0.076 - 8 (g/l)	350
	TFTUR-L00/AU	7x70 ml	7x20 ml				2450
KIT for AU®400-640-2700-5400	TFTUR-H00/AU	1x70 ml	1x20 ml	36 months	Serum and plasma	0.076 - 8 (g/l)	280
	TFTUR-L00/AU	7x70 ml	7x20 ml				1960
KIT for AU®5800	TFTUR-H00/AU	1x70 ml	1x20 ml	36 months	Serum and plasma	0.076 - 8 (g/l)	467
	TFTUR-L00/AU	7x70 ml	7x20 ml				3267

CALIBRATORS

KIT 5 LEV	MPREK-000	5x1 ml	24 months
-----------	-----------	--------	-----------

CONTROLS

H	MPCOX-002	1x2 ml	24 months
M	MPCON-002	1x2 ml	24 months
L	MPCOS-002	1x2 ml	24 months



Your expert in specific proteins

(*) Shelf Life :

DiAgam provides to distributors a minimum of **12 months** (except Ferritin and Lp(a): 10 months) .
The time period written in this document shows the maximum shelf life time after manufacturing.

() Sample :**

DiAgam may provide some applications for other samples, such as CSF, Urine, Veterinary samples etc.... Please contact your distributor or us directly at mail@diagam.com or dial +32 68 55 14 82.

(*) Analytical range :**

For general information purposes only. More details can be found in the package insert (instructions for use). Please contact your distributor or us directly at mail@diagam.com or dial +32 68 55 14 82 in order to get the updated data.

(**) Tests :**

Amount of tests possible by kit. May vary from an instrument to another one.



Medical device for in vitro diagnostics.

Contact information:

for orders, invoicing and technical queries, we kindly recommend you to use our general e-mail address that is mail@diagam.com.



DIAGAM SA, Rue du Parc Industriel, 7822 Ghislenghien, BELGIUM

© DiAgam. 2021. All rights reserved. All product names, registered trademarks, company names in this document remain the property of their respective owners. For general information purposes only. More details can be found in the package insert (instructions for use) and labelling. Not for the US market except for research use only.